




# NT-H2-PL1000

## Premium Line Electrochemical Hydrogen Sensor

D55397 rev.0 dated 03/05/2024

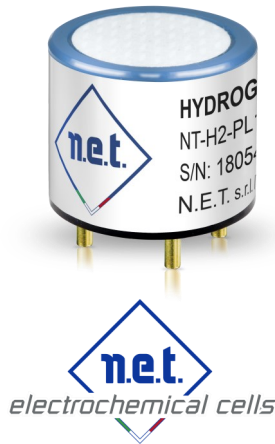

### Key Features

The NT-H2-PL1000 is a new Premium Line electrochemical gas sensor with 3 electrodes for the detection of Hydrogen in a variety of gas detection applications. Exhibiting high performance with excellent resolution for low-level ppm detection as well as stability and output signal, this compact sensor (20.4 mm diameter) is suitable both for portable and fixed gas detection instruments.

The porous electrode technology enables accurate gas detection with high sensitivity. The mechanical design of the sensor gives optimum gas diffusion characteristics, and the hermetically sealed enclosure prevents costly electrolyte leakage.

### NET Premium Line Electrochemical Cells

The European Standard EN 45544-2 (Workplace atmospheres. Electrical apparatus used for the direct detection and direct concentration measurement of toxic gases and vapours. Performance requirements for apparatus used for exposure measurement) specifies the performance requirements for electrical apparatus used for the direct detection and direct concentration measurement of toxic gases and vapours in workplace atmospheres, including sensors. This standard provides a consistent approach and framework for the assessment of performance criteria to manufacturers, test laboratories and users of apparatus.


But, the standard states, "It is the manufacturer's primary responsibility to ensure that the apparatus meets the requirements laid down, including environmental influences

which can be expected to affect performance".

With this in mind, N.E.T. has designed its PREMIUM LINE: a range of electrochemical cells to exceed all the performance requirements of EN 45544-2 – including upper and lower limit of measurement, deviation of the measured values in clean air and in standard test gas, deviation of the measured values at all temperatures, pressures and at any humidity, time of response (t90, t50), time of recovery (t10, t50), over-range and stability.


The Premium Line is manufactured exclusively for N.E.T. in Japan and includes sensors for CO, NO, NO2, H2, H2S, SO2, HCl, Cl2, NH3 (available in 4 different ranges) and the new H2S-HT and CO-HT cells for high temperatures.

### Mechanical specifications

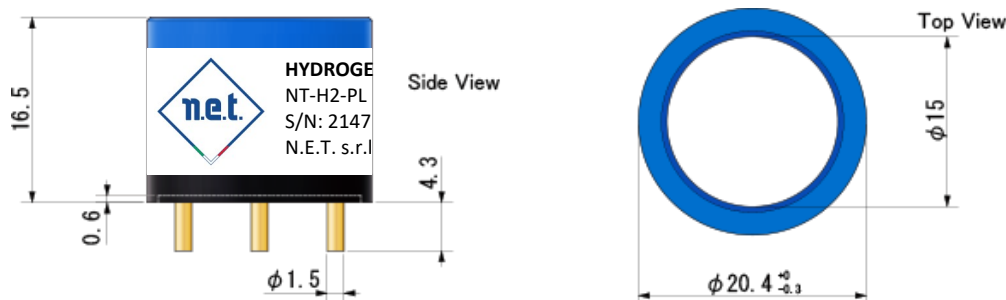

All dimensions are in mm with a tolerance of +/- 0.1 mm unless stated otherwise

## Pinout

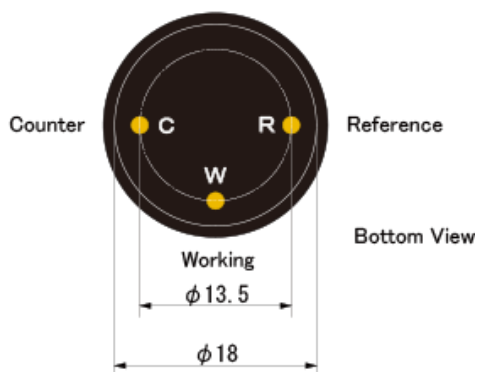

## Product specifications

Technical Specifications	Detection Gas	Hydrogen
	Detection Range	0 ~ 1000 ppm
	Maximum Overload	2000 ppm
	Output Signal	25 +/- 10 nA/ppm
	Repeatability	< +/- 2 %
	Resolution	1 ppm
	Typical Baseline Range (pure air)	< +/- 5 ppm
	Typical Response Time (t90, 20□)	30 seconds
	Typical Baseline Shift (- 40 ~ 40□)	< +/-5ppm(typical)
	Expected Life Time	< 2%/month
	Weight	4.5 g (approx.)
Operating conditions	Operating Temperature	> 2 years
	Operating Humidity	-30 ~ +50°C
	Operating Pressure Range	15 ~90 % RH
	Recommended Load Resistor	1atm +/- 10 %
	Bias Voltage	Not required
	Position Sensitivity	None
	Recommended Storage Temp.	0 ~ +20°C
	Storage Life	Less than 6 months
Warranty	2 years on mechanical defects only	


Performance data conditions: 20°C, 50%RH and 1013mBar

## Typical cross sensitivities

Gas	Test Gas Concentration (ppm)	Typical CO Concentration Equivalent (ppm)
Hydrogen	100	100
Carbon Monoxide	300	80
Hydrogen Sulfide	10	0
Sulphur Dioxide	20	0
Carbon Dioxide	5	0
Nitrogen Dioxide	10	0
Nitric Oxide	50	0
Ethylene	100	40
Ethanol	200	0
Ammonia	100	0


**Important note:** The values above are typical values and should not be used as a basis for cross calibration. Cross sensitivities may not be linear and should not be scaled either. Above data based on gassing for 5 minutes using test equipment. Should be noted some cross interference break through will occur if gas is applied for a longer period of time.

## Linearity

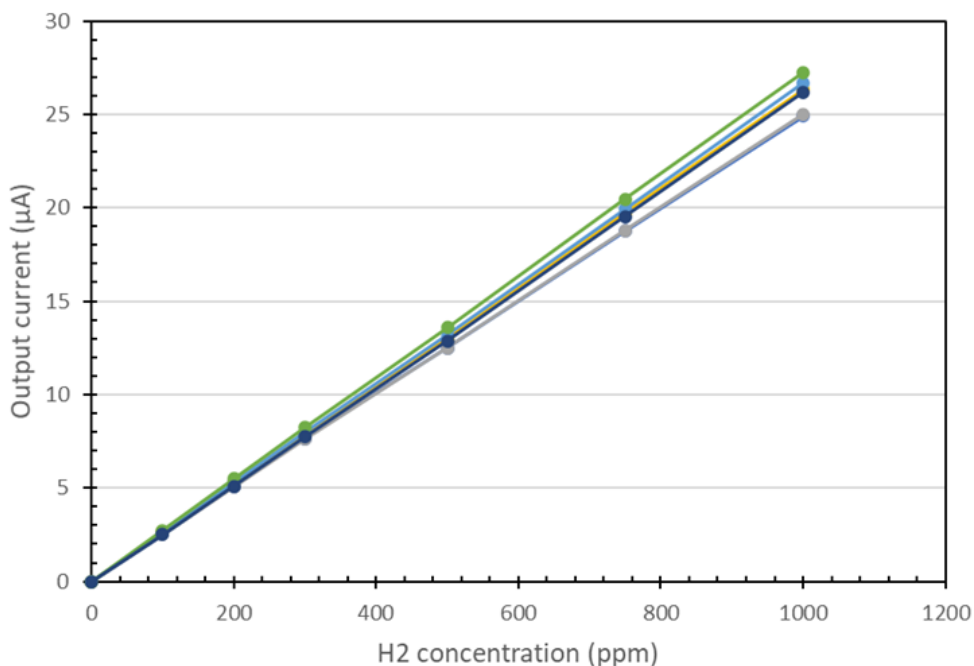


Linearity characteristics of NT-H2-PL1000 (25°C)

## Response and Recovery

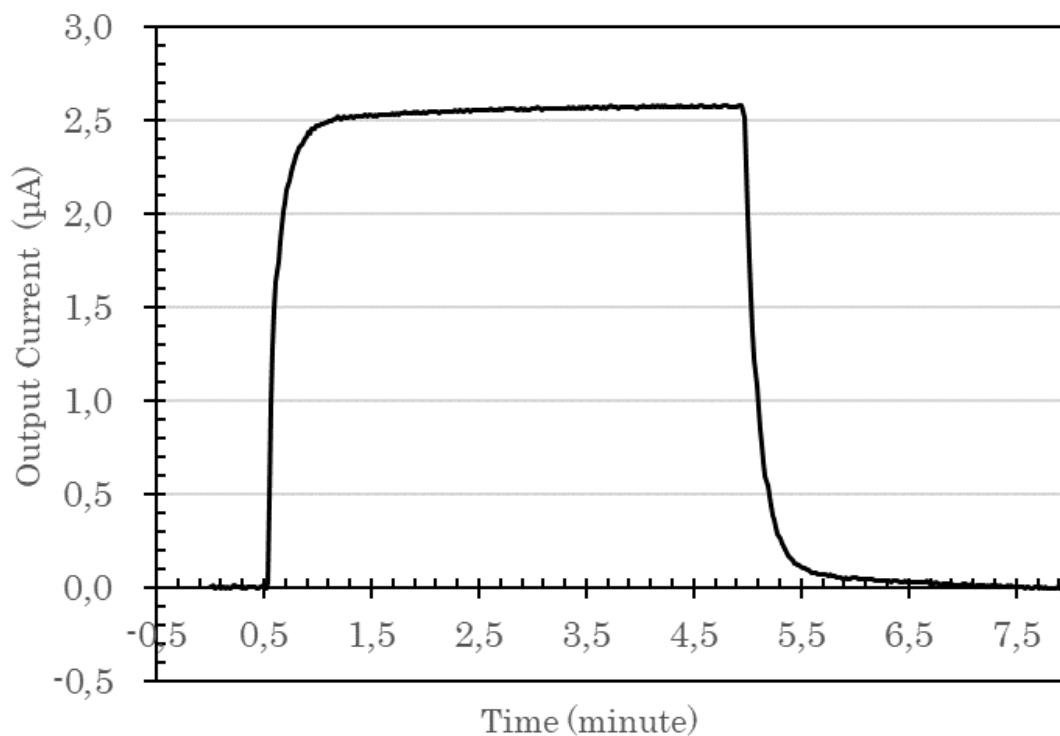


Response and Recovery characteristics of NT-H2-PL1000 — (H2:100ppm, 20°C)

## Baseline shift

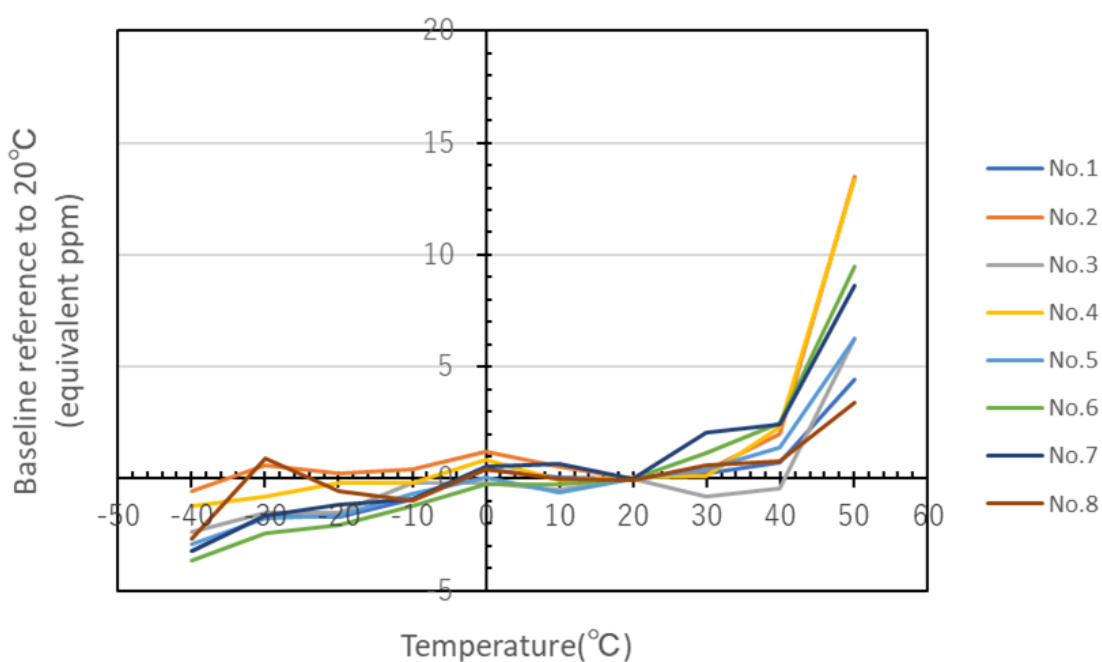


Baseline shift of NT-H2-PL1000

## Temperature dependency

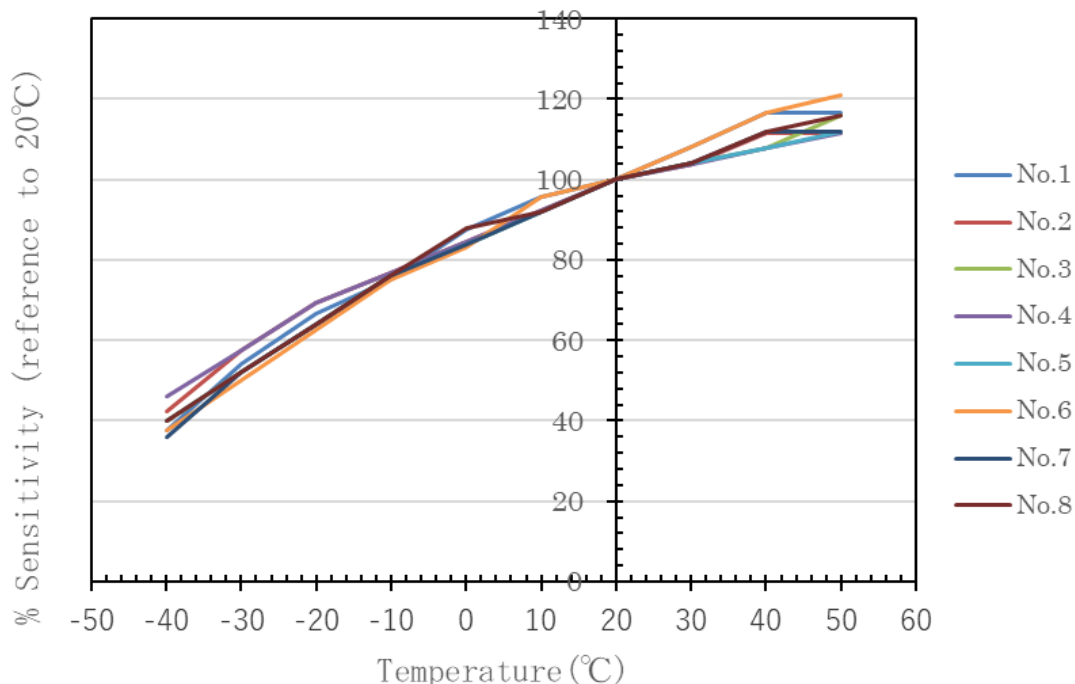

## Recommended Circuit Diagram

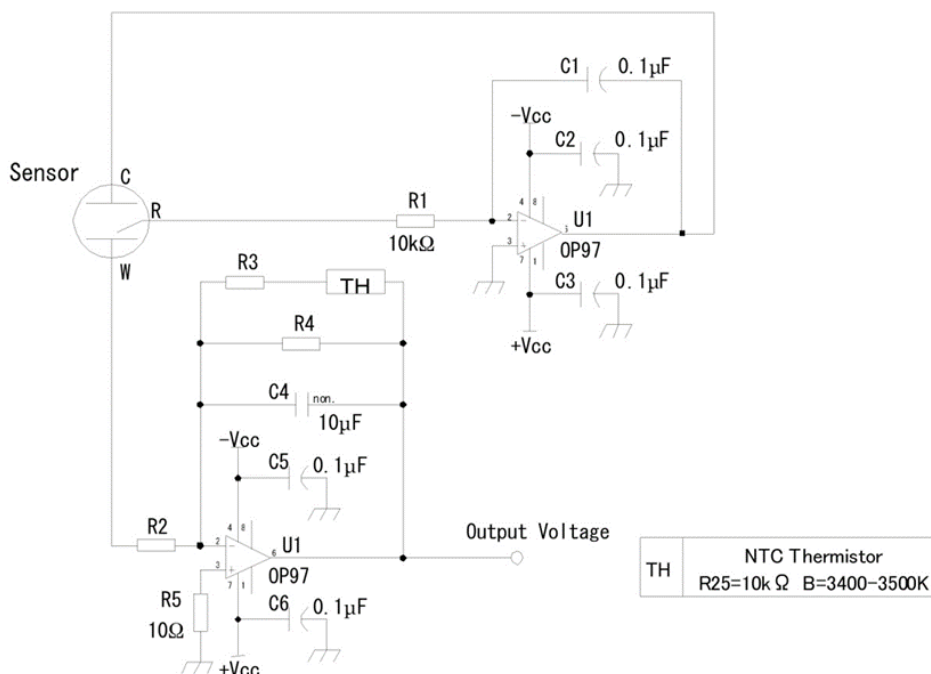

In the circuit, R2=10 Ω, R3=12.1 kΩ and R4=18.2 kΩ. The temperature dependence of the sensor is compensated by NTC thermistor that has 3435K of B constant. Other thermistor can be used, if the B constant is around 3500K and the resistant value (R25) is 10 kΩ.

## Warranty and warning

- Use within specified conditions.
- It is customer's responsibility to confirm that device can be used under actual conditions of use without any problems.
- Calibration is required to maintain correct sensitivity. It is necessary approximately once every six months to one year.
- Sensor characteristics must be measured in clean air without noise gases.
- Electrode pins must be correctly connected. Wrong connection does not allow correct functions.
- Do not apply voltage directly to electrode pins.
- Do not bend pins.
- Do not solder to electrode pins directly. Use exclusive sockets.
- Do not use contact grease on electrode pins.
- Do not put excess strength on electrode pins.
- If sensor housing is damaged or scratched, do not use sensor.

**N.E.T. has a policy of continuous development and improvement of its products. As such the specification for the device outlined in the data sheet may be changed without notice. In case of modification of the product, N.E.T. disclaims all liability.**

**No part of this publication may be reproduced, distributed, or transmitted in any form or by any means, including photocopying, recording, or other electronic or mechanical methods, without the prior written permission of N.E.T. For permission requests or technical support please contact or write to the address below:**

**N.E.T. SRL**  
**Via Campania, 5 | 20006 | Pregnana Milanese | MI | Italy**  
**T +39.02.9354.4190**  
**E [info@nenvitech.com](mailto:info@nenvitech.com)**  
**[www.nenvitech.com](http://www.nenvitech.com)**